

NOV 09 2009

Supervisor/Operator Performing the Verification Procedure:

DataMaster edm S/N 130289 ✓

Name Byron D. Redburn

ID# 2087 Date 10/31/2009 ✓

A

Agency Nome PD

Phone # 943-5262

Instrument Location Nome PD ✓

B

Alco S/N X801548 ✓ Target Value .079 High Pressure 525

Alco Test Values

.079
1st Alco ✓

~~.080~~ .078
2nd Alco
11-09-09
CMB

Signature B.D. Redburn ✓

(OVER)

(Do Not write in the area below)

CMB
11/14/09


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 3rd day of Dec., 2009.

Carolyn M. Noland
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office
BT9 06/03

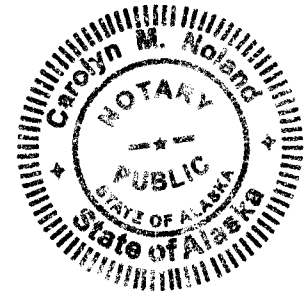

ALASKA DEPARTMENT OF PUBLIC SAFETY
Bureau of Criminal Investigation
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster edm S/N 130289

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130289

OCTOBER 31, 2009

OPERATOR'S NAME:

REDBURN BYRON D

OPERATOR'S NUMBER: 2087

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/NI:

A

O.L. #: A

DEPT/AGENCY: ONEI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: .079

ALCO S/N: K301548

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 30.43 in ✓
ALCO TARGET .000 13:10
BLANK TEST .000 13:10
INTERNAL STANDARD VERIFIED 13:10
ALCO TV 30.43 in .079 ✓ 13:11
BLANK TEST .000 13:12
SUBJECT SAMPLE .000 13:13
BLANK TEST .000 13:13
ALCO TV 30.43 in .079 ✓ 13:14
BLANK TEST .000 13:14

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130289

OCTOBER 31, 2009

TIME 13:06

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 41c
BAROMETER: 30.43 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~